AIR CUSHION AND PUMP SYSTEM (EP-C)

Quick Guide

1. POWER UP

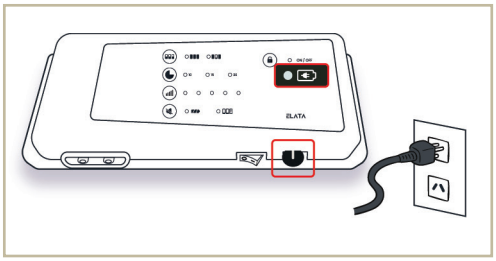

Connect the power cable to pump & wall outlet. Charge until battery light turns off

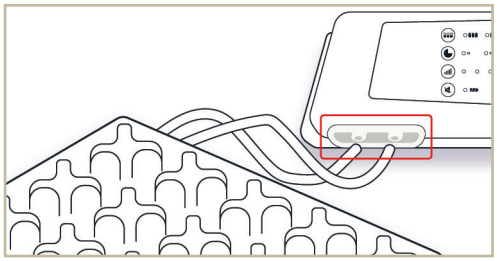

Connect the pump to cushion tubes

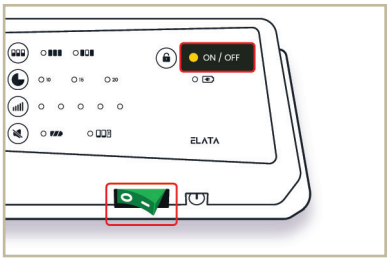

Press Power Switch. The On/Off indicator should light yellow

2. SELECT SETTINGS

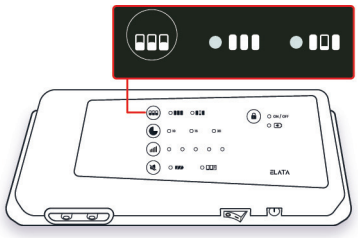

- *The Static Mode inflate all cells in your cushion*
- *The Alternating Mode inflate and deflate the cells in your cushion alternately*

If Alternating mode, is selected you can set the cycle time. cycle time selected will light up green

10 15 20

Select the Pressure level between 1 - 5 based on the approximate user weight

Pressure Setting	1	2	3	4	5
Approx. User Weight	60kg	80kg	100kg	160kg	220kg

It is recommended that the user starts at the pressure setting closest to their recommended weight and then adjust it lower or higher based on their comfort

3. START THERAPY

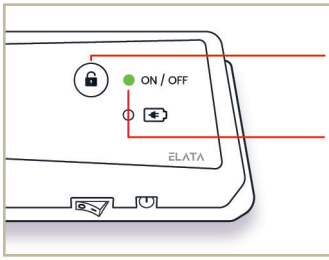

Hold Start/Stop for 2 sec.

The ON/OFF light will turn from yellow to green

Adjust mode, time, or pressure at any time based on comfort

TROUBLESHOOTING

If you hear a beep coming from your Elata Air Cushion System, it will indicate the following:

- *Indicates low battery warning*
- *Indicates low pressure warning*

Press Mute key to silence alarms